

NEW! Fisher Chemical UHPLC-MS Solvents

Ultra high purity solvents linked directly to the sensitivity of the mass spectrometer that minimizes chromatographic interferences.

Fisher Chemical has developed a new solvent grade, UHPLC/MS Optima™, for mobile phases targeting trace analysis by UHPLC/MS.

These ultra-pure solvents will provide a very low mass noise level in both positive and negative mode ionization, minimal metal ion content, and very low UHPLC/UV response using photo diode array detection. Fisher Chemical's high purity solvents are specifically qualified for UHPLC-MS and offered in Acetonitrile, Methanol, and Water.

Solvent	Pack size	Packaging	Catalog Number
Acetonitrile	1L	Borosilicate Glass	A956-1
Methanol	1L	Borosilicate Glass	A458-1
Water	1L	Borosilicate Glass	W8-1



Why Fisher Chemical UHPLC-MS Optima™ Solvents?

- New solvent specification based on S/N ratio of the propazine product ion from MS/MS fragmentation.
Benefit: The solvent quality of UHPLC-MS Optima solvents is linked directly to the sensitivity of the detector (mass spectrometer); unique specification for the chemical industry.
- 0.1 micron filtration for Acetonitrile and Methanol, 0.03 micron filtration for Water.
Benefit: Submicron filtration ensures minimal clogging of instrument, columns and check valves.
- Reduces significantly the leaching of metal cations (Na⁺ and K⁺).
Benefit: Low metal content in mobile phase solvents minimizes formation of metal ion adducts.
- Fisher Chemical UHPLC-MS solvents have an LC-UV Gradient Suitability specification which is tested in the full 200–400 nm range.
Benefit: Mobile phase solvents have minimal UV-absorbing impurities providing customers with smooth baselines with minimal interference (a smooth baseline in chromatogram with minimal interference).
- Convenient 1 L bottle borosilicate glass design accommodates mobile phase as bottle can sit on top of UHPLC-MS instrument.
Benefit: Ease of use directly on instrument.

Did You Know



Ultra High Performance Liquid Chromatography (UHPLC) performs separations 5 to 10 times faster than conventional HPLC by employing sub-2 µm diameter particles? The 1-2 second peak widths and relatively high separation efficiency of UHPLC are more competitive with capillary GC, making UHPLC-MS an attractive method for illicit drug analysis.

Fisher Chemical UHPLC-MS Optima™ solvents for mobile phases support interference-free analytical work:

UHPLC-UV Gradient Suitability Test

UHPLC-UV Specification



Peak height with PDA (200–400 nm) is < 2 mAU.

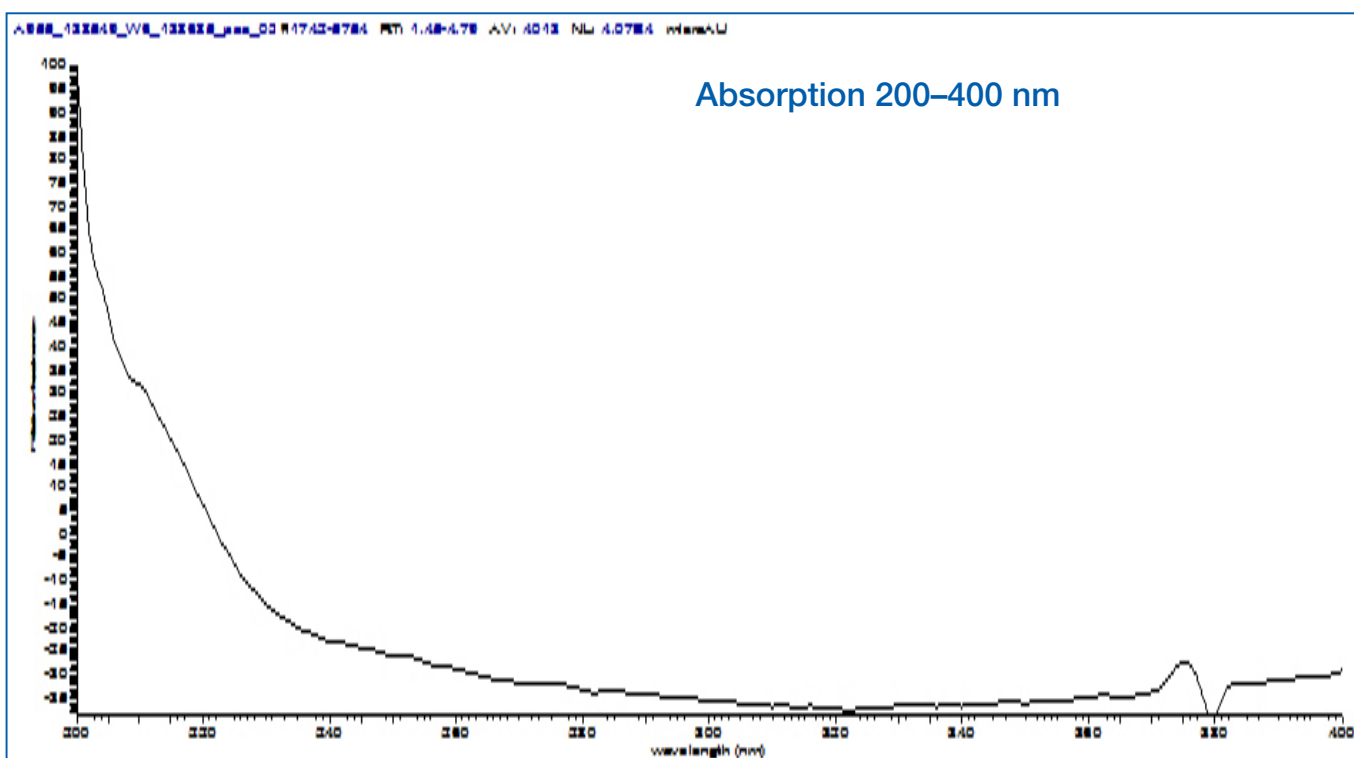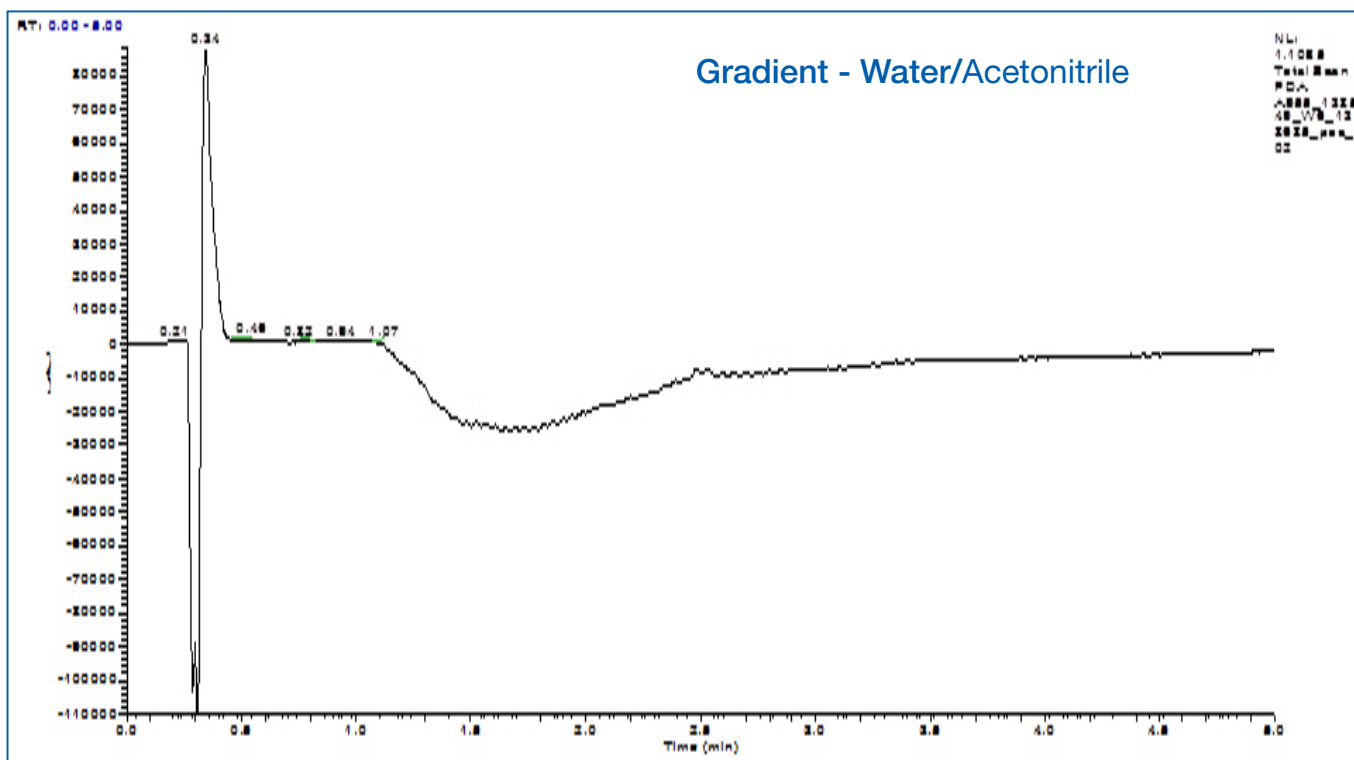

UHPLC-MS/MS of 250 ppt Propazine

UHPLC-MS/MS Specification:



Signal-to-noise ratio of Propazine product ion peak m/z 188 is > 10 .

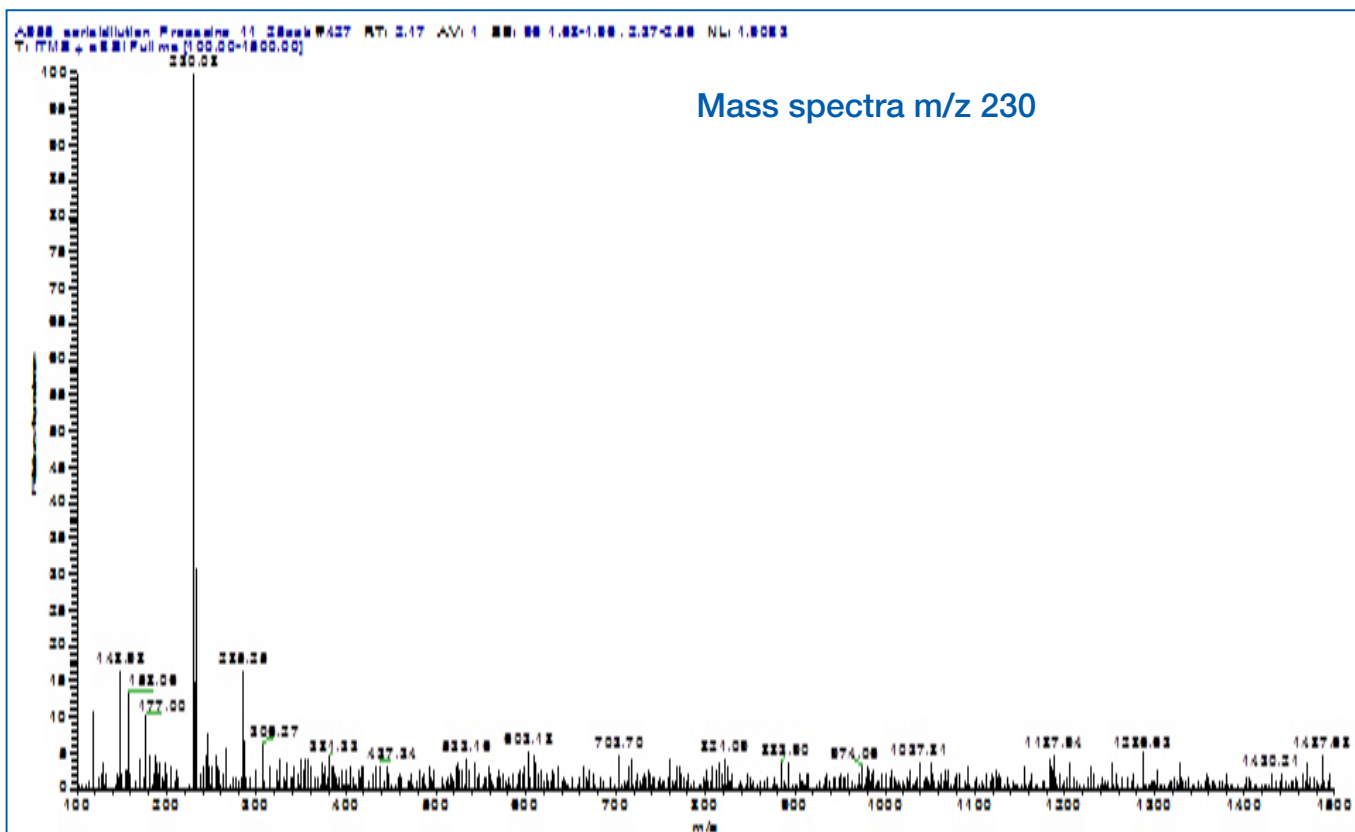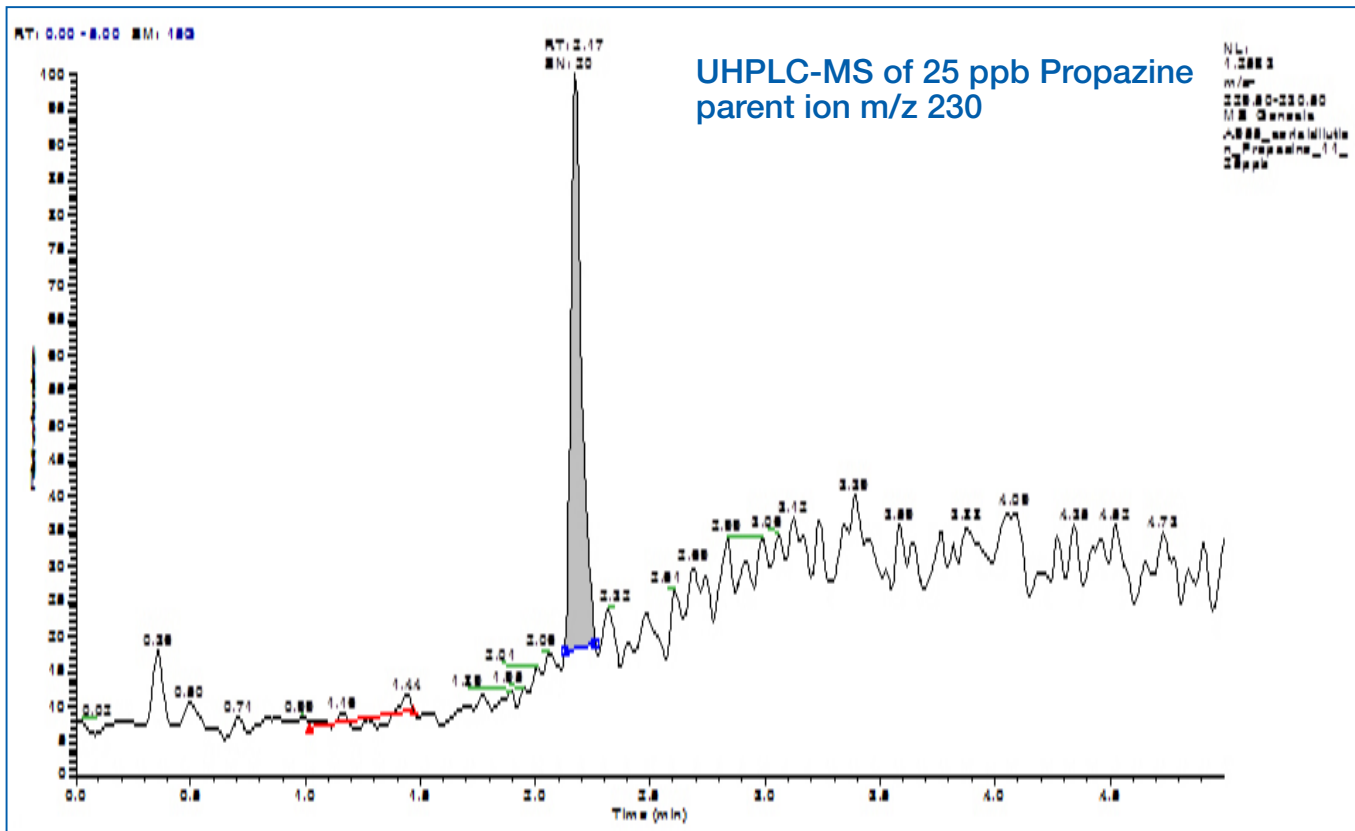

UHPLC-MS Gradient Suitability Test

UHPLC-MS Specification:

In positive mode ionization, any eluted peak height is < 25 ppb Propazine parent ion m/z 230 in full scale TIC and EIC.

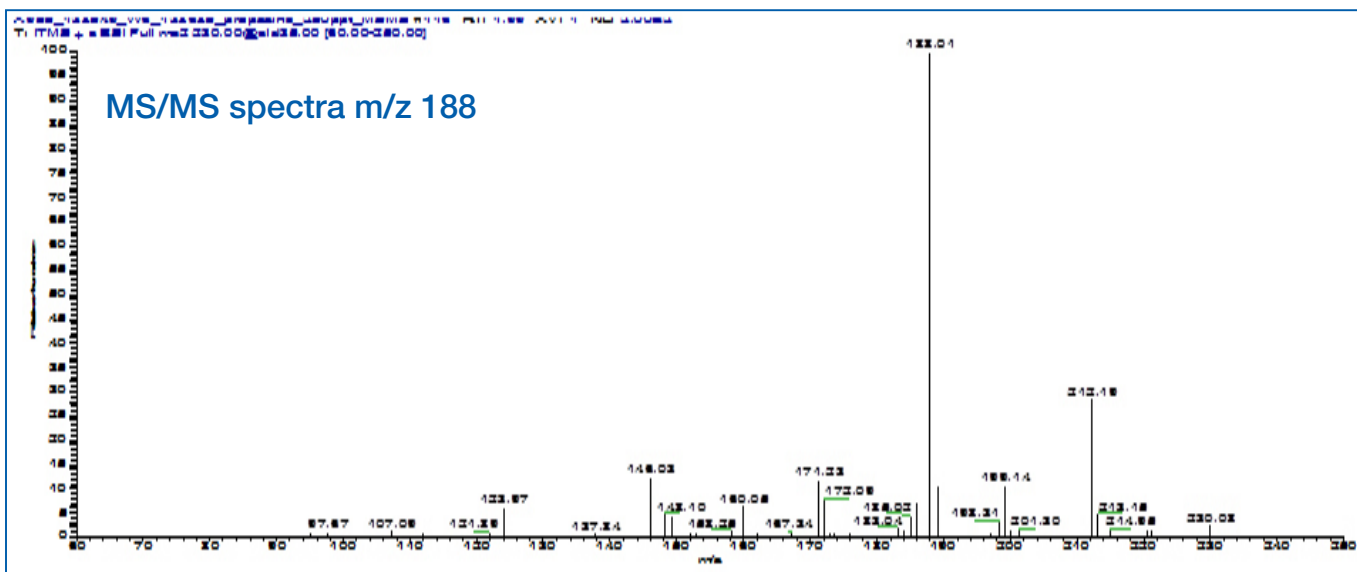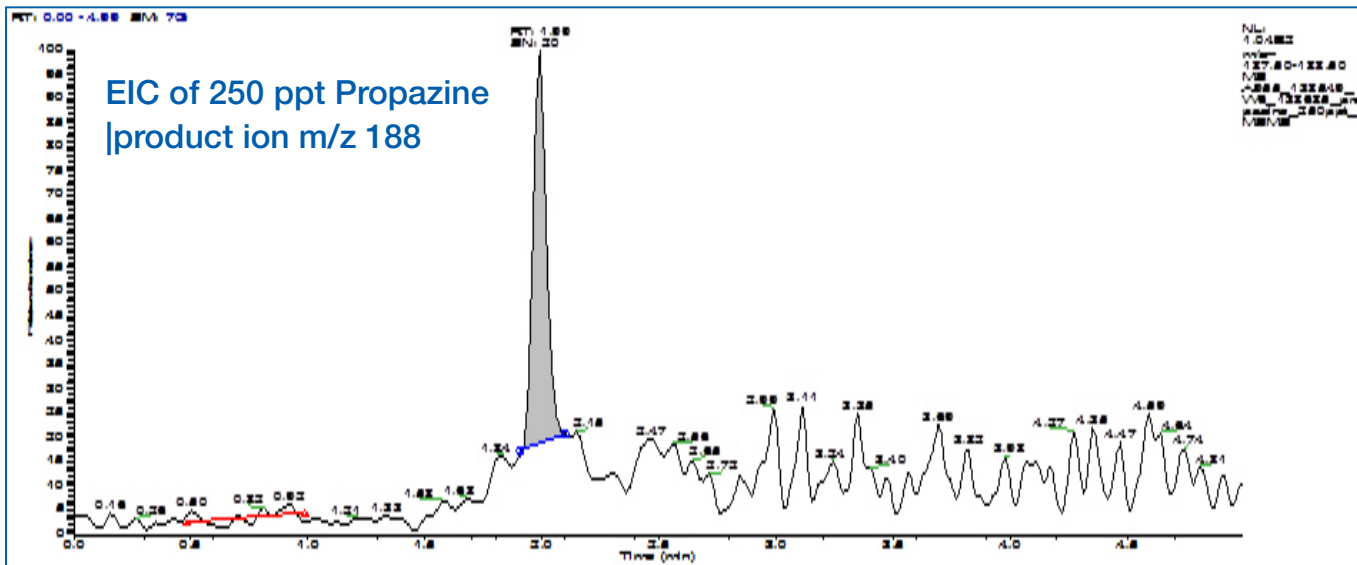

To place an order, contact your local distributor.



©2015 Thermo Fisher Scientific Inc. All rights reserved.
All trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries.

Thermo Fisher Scientific
ENA 23, Zone 1, nr 1350
Janssen Pharmaceuticaan 3a
2440 Geel
Belgium
www.acros.com